HeartStart OnSite Defibrillator

QUICK REFERENCE

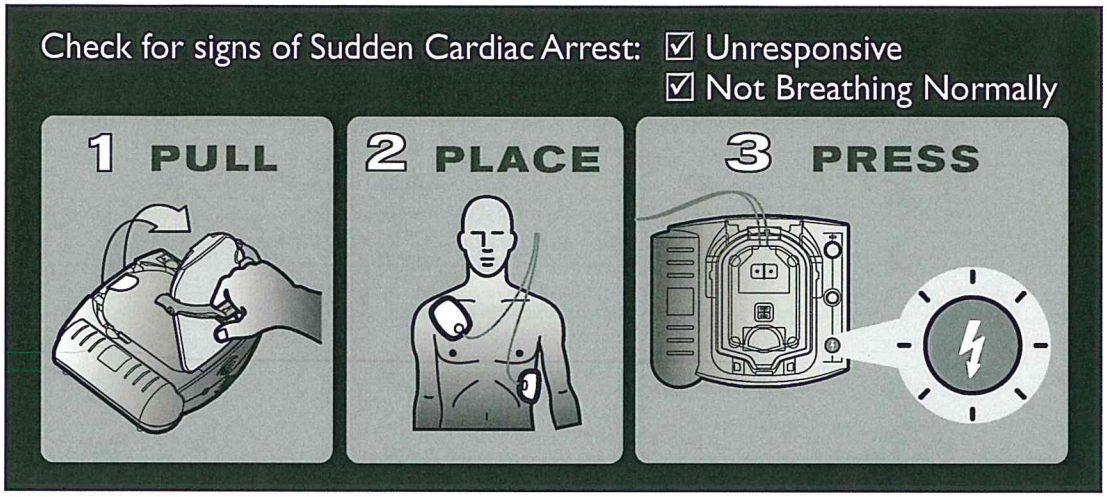

PHILIPS MEDICAL SYSTEMS

STEP 1: PULL THE GREEN HANDLE

Turn on the OnSite by pulling the SMART Pads Cartridge's green handle.* Remove the hard cover from the pads cartridge and set it aside. Remain calm and follow the OnSite's instructions.

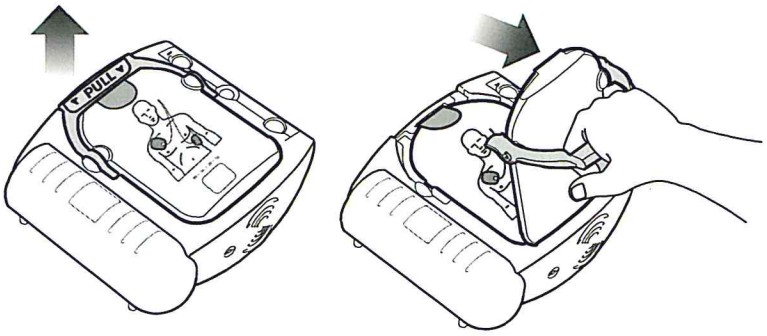

The OnSite starts by directing you to remove all clothes from the patient's chest. If necessary, rip or cut off the clothing to bare the person's chest

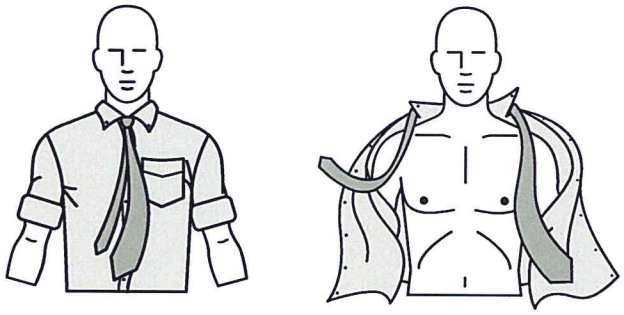

* You can also turn on the OnSite by pressing the green On/Off button.

STEP 2: PLACE THE PADS

Pull the tab at the top of the pads cartridge to peel off the film seal. Inside are two adhesive pads on a plastic liner. Remove the pads from the cartridge.

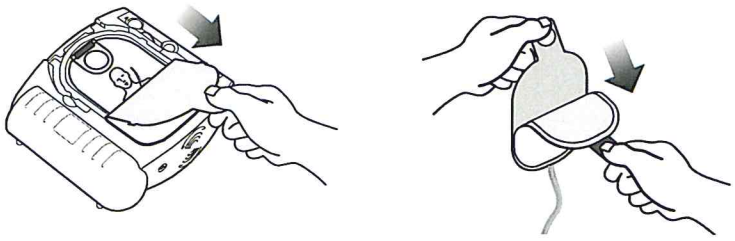

Peel one pad off the liner. Place the pad on the patient's bare skin, *exactly as shown in the picture on the pad.* Press the pad down firmly. Then repeat this with the other pad. Be sure the pads have been removed from the liner before placing them.

Where to place pads on adults and children over 25 kg/55 pounds or 8 years old (anterior-anterior).

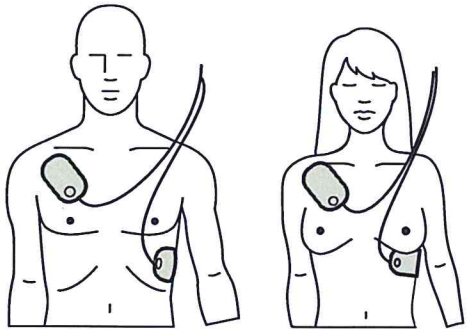

Where to place pads on infants or children under 25 kg/55 pounds or 8 years old (anterior-posterior).



STEP 3: PRESS THE SHOCK BUTTON

As soon as the OnSite detects that the pads are attached to the patient, it begins analyzing the patient's heart rhythm. It tells you that no one should be touching the patient, and the Caution light ⚠ begins flashing as a reminder.



If a shock is needed:

The Caution light ⚠ goes from flashing to solid, the orange Shock button ϟ starts flashing, and the OnSite tells you to press the flashing orange button. Before you press the button, make sure no one is touching the patient. When you press the Shock button, the OnSite tells you that the shock has been delivered. Then the OnSite tells you it is safe to touch the patient, instructs you to begin CPR, and invites you to press the flashing blue i-button ⓘ for CPR Coaching if desired.

If a shock is not needed:

The OnSite tells you it is safe to touch the patient and instructs you to perform CPR if needed. (If CPR is not needed – for example, if the patient is moving or regaining consciousness – follow your local protocol until emergency medical personnel arrive.) Then the OnSite invites you to press the flashing blue i-button ⓘ for CPR Coaching, if desired.



For CPR Coaching:

Press the flashing blue i-button ⓘ during the first 30 seconds of the patient care pause to activate CPR Coaching.* (If the Infant/Child SMART Pads Cartridge is inserted, CPR Coaching will provide coaching for infant/child CPR.) When the pause is over, the OnSite tells you to stop CPR, so it can analyze the patient's heart rhythm. The motion caused by CPR can interfere with analysis, so be sure to stop all motion when instructed.

* The default configuration for the OnSite provides CPR Coaching when you press the i-button in this situation; however, the default setting can be revised by your Medical Director using Philips software available separately. See Appendix F for more information.